

Plastic Mannequin-Based Robotic Telepresence for Remote Clinical Ward Rounding

Victor O. Matthews, Segun I. Popoola, and Aderemi A. Atayero, *Members, IAENG*

Abstract—Mobile robotic telepresence is a potential solution to addressing the problem of access to quality healthcare delivery in rural areas. Despite the availability of this system in its different forms, the capital and operating costs are unaffordable for people living in rural areas, particularly in emerging economies. In this paper, the authors reduced the cost of mobile robotic telepresence solution for remote ward rounding using plastic mannequin and solar photovoltaic technology. An IP camera was fixed in each of the eye sockets of the plastic mannequin. These cameras are connected to a mini-computer embedded in the plastic mannequin. A Wi-Fi module establishes an Internet connection between remote physicians and rural healthcare facilities. In addition, most of these communities are not even connected to the power grid. Therefore, the system is powered by a solar photovoltaic energy source to provide a cheap and reliable power system. Another unique feature of this solution is that it gives the patient a better impression of the physical presence of a physician. This development will increase the adoption of robotic telepresence for remote clinical ward rounding in developing countries.

Index Terms—mobile robotic telepresence; plastic mannequin; solar photovoltaic; ward rounding

I. INTRODUCTION

ADVANCES in ICT technologies can be readily exploited to solve the challenges confronting the provision of quality healthcare delivery in rural areas. There is usually shortage of qualified medical experts in remote health facilities. The cost and risk associated with travelling over a long distance to seek medical attention in urban centers is also high. Overdependence of rural dwellers on health facilities in the cities can increase mortality rate in cases of emergency. It is, therefore, necessary to leverage available technologies to provide urgent solution to this problem.

Telepresence is one of the innovative solutions for telemedicine applications. The World Health Organization (WHO) [1] defined telemedicine as “*the delivery of health care services, where distance is a critical factor, by all health care professionals using information and communication technologies for the exchange of valid information for diagnosis, treatment and prevention of disease and injuries, research and evaluation, and for the continuing education of health care providers, all in the interests of advancing the health of individuals and their*

communities”. Communities with inadequate healthcare infrastructure and personnel can adopt the use telemedicine applications to augment their deficiencies. Geographical barriers are commonly encountered when trying to connect patients to specialists in referral hospitals that are not in the same physical location [2]. Real-time video telecommunication capabilities of telemedicine [3] will assist health workers, medical consultants and specialists to deliver health care services to patients living in remote areas. The service may be in form of direct patient care, health education, and clinical consultation in critical care, transmission of dermatologic or radiologic images, or real-time video distant-monitoring support in the intensive care unit [4].

Several telepresence initiatives have been developed for health care applications. Remote tele-consultative service offered in [5] using a two-way audiovisual link produced a better clinical and educational effect than the telephone [6]. eICU [7], a dedicated facility designed for intensive care unit, allowed a consultant to supervise and monitor patients in different locations at the same time, reducing mortality and cost [8, 9]. Telemedicine have been applied for trauma and neurology consultative services where there are no resident specialist [10-14]. Despite the advances in this technology, its adoption among underserved population has been very limited. Major hindrances include the problems of complex human and cultural factors [15], lack of proof of economic benefits and cost-effectiveness, and legal considerations [16-18].

Robotic telepresence is a form of telepresence that creates an impression of the physical presence of an object at a remote location. This feature is accomplished through a mobile robotic mechanism with real-time audiovisual communication capabilities [19-26]. Considering the high level of extreme poverty in emerging economies, most of the available solutions designed to overcome this challenge are relatively unaffordable for deployment in this region. Also, the unreliability of power grid in rural areas where most communities are not even connected, will eventually hamper the sustainability of the whole system.

In this paper, the authors reduced the cost of mobile robotic telepresence solution for remote ward rounding using plastic mannequin and solar photovoltaic technology. An IP camera was fixed in each of the eye sockets of the plastic mannequin. These cameras are connected to a mini-computer embedded in the plastic mannequin. A Wi-Fi module establishes an Internet connection between remote physicians and rural healthcare facilities. In addition, most of these communities are not even connected to the power

Manuscript received March 17, 2017; revised March 28, 2017.

V. O Matthews, S. I. Popoola, and A. A. Atayero are with the Department of Electrical and Information Engineering, Covenant University, Ota, Nigeria (corresponding author e-mail: segunpopoola15@gmail.com).

grid. Therefore, the system is powered by a solar photovoltaic energy source to provide a cheap and reliable power system. Another unique feature of this solution is that it gives the patient a better impression of the physical presence of a physician. This development will increase the adoption of robotic telepresence for remote clinical ward rounding in developing countries.

II. MATERIALS AND METHOD

The plastic mannequin-based telepresence is a robotic system that is remotely controlled using a web-based software application that runs on the Internet. The hardware part of the system include two IP cameras, mini-computer, wireless network transceiver, and audiovisual system. These are enclosed in a plastic mannequin as shown in Figure 1. This computer humanoid approach is employed to give a better impression of the physical presence of the medical consultant to the patient. The utilization of a plastic mannequin, which are relatively cheap, will significantly reduce the overall cost of the robotic system. To fully maximize the advantage of this method, the plastic head can be remolded to depict the face of the medical practitioner attending to the patient from a remote location. The plastic mannequin is dressed in the regular attire of health worker on duty.

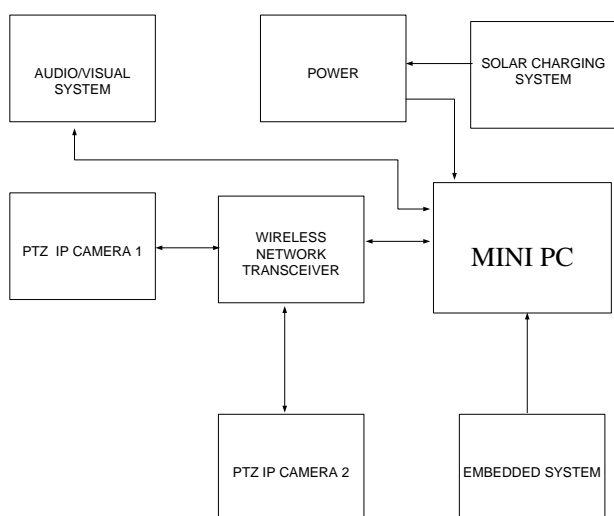


Figure 1: Block Diagram of Plastic Mannequin-Based Telepresence

An IP camera is a network-based camera of high definition with the capability to pan, tilt, and zoom, and transmits data over the Internet. It enables easy access and real time human interactions when the integrated web server is connected to the Internet. There is a high degree of freedom of movement that enables views from different directions and multiple angles. This makes it ideal for continuous object tracking. Users can conveniently zoom in on a farther object for better view. In practice, this type of camera produce irregular response time to control commands, low frame rate, irregular frame rate due to network delays, varying field of view that results from panning, tilting, and zooming, and different scales of objects. However, with the adaptive fuzzy particle filter algorithm proposed in [27] the displacements in the image plane between two consecutive frames is reduced, and the

detected target location is near to the ground-truth. By this, the camera exhibits a better precision on focus.

Of the two cameras fixed into the eye sockets of the mannequin, one is intended to enable remote access for a distant-consultant while the other is reserved for a specialist. This is aimed at facilitating professional collaboration to boost the quality of healthcare delivery in the rural areas of developing nations. The IP cameras are securely accessible to the health professionals via a web server application.

A low-cost, energy-efficient IP camera is made up of a video pre-processing unit, an H.264 encoder, and an embedded streaming server [28]. The video data is acquired and properly formatted by the video pre-processing unit. The output of the pre-processing unit is compressed with H.264 baseline encoding tools, and a continuous flow of data is ensured by the streaming server for the Internet video communication. Based on cheap and power-efficient Blackfin Digital Signal Processor (DSP) and ARM9 processors employed in the encoder and the streaming server, and optimal use of the DSP resources, the IP camera delivers Common Intermediate Format (CIF) or Video Graphic Array (VGA) size of real-time video clips directly to the Internet with high Peak Signal-to-Noise Ratio (PSNR) quality and low bit rates. This improves video quality at reduced bandwidth, and makes the system more reliable.

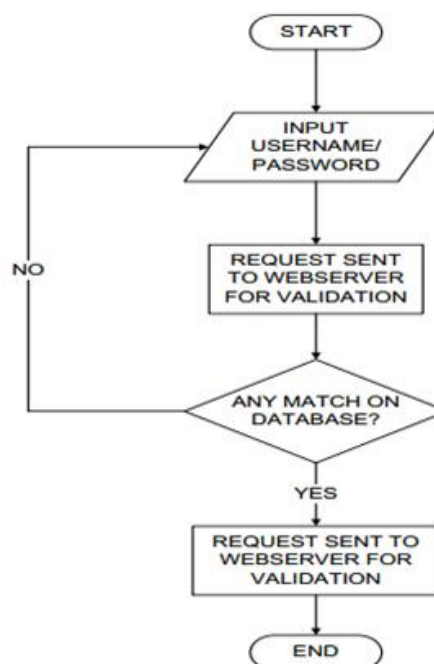


Figure 2: Flow Chart of Web Server Operation

For the audiovisual sub-system, a microphone is fixed on the neck section of the mannequin. With this, the remote users can easily pick up acoustic signals from the clinical ward for effective communication. The microphone is sensitive to vibrations, thus providing good acoustic quality. The well-perforated chest part of the mannequin houses the speaker. A four-wheel movement support is designed at the base carriage, and operated by a 12-volt DC electric motor. The program codes of the system is loaded to a mini-computer located within the plastic mannequin.

Raspberry Pi, an 85.60 mm x 53.98 mm x 17 mm single-

board computer, performs computations with much less power consumption compared to desktop computers, laptops, tablets and smart phones [29]. The low-cost mini-computer has general-purpose input/output universal serial board (USB) ports (1 to 4) for connections to external devices. Latest release, Raspberry Pi 3 Model B, is equipped with RAM (256 MB to 1 GHz), on-board Wireless LAN (Wi-Fi IEEE 802.11n), an 8P8C Ethernet port and Bluetooth. It also features a central processing unit (CPU) with speed range of 700 MHz to 1.2 GHz, and a graphic processing unit (GPU). The price of the advanced model varies between US \$20-35. The operating system and application programs are stored in secured digital (SD) cards of SDHC or micro-SDHC sizes. The system also has a HDMI and composite video output alongside a 3.5 mm audio jack for audiovisual communications. The mini-computer is connected to the Internet via a Wi-Fi communication link established between a high-speed access point and Wi-Fi adapter of the mini-computer. Remote users can easily log in to the system using different platforms such as smart devices, desktop computers, laptops, PDAs etc.

Few community health workers available at rural health facilities will assist the medical experts in collecting vital health information and records of patients. The system allows real-time audiovisual communication between the medical professionals, the community health workers, and the patients. The pan-tilt-zoom capability of the IP network cameras enables the remote consultant and specialist to gain a complete view of the hospital ward, and if necessary zoom in to focus on a particular part of the body of the patient with no assistance from the community health workers.

A client-server model was used for the web server and Hypertext Transfer Protocol (HTTP) forms the webpages. This module links the remote user to the robotic telepresence system. The Apache webserver runs on a dedicated computer. An obstetricians based in any of the developed countries, say United States of America, with a pre-assigned authentication code can log in to the electronic platform to attend to different patients at different rural health facilities. Several other specialists/consultants (pediatricians, anesthesiologists, critical care medicine specialists, gynecologists etc.) can also attend to patients in different wards of remote clinics during routine ward rounding. Data signal is transmitted from the smart device or internet-enabled personal computer of the remote medical experts and it is routed through the internet cloud to connect to the system. With a reliable internet connection setup at the rural clinic, the specialist/consultant gains remote control of the robotic system with ease. The movement of the mannequin is guided by the audio-visual information that is clearly available to the user. The user communicates effectively with the assisting community health workers as well as with the patients through an open-source remote viewer software. This publicly available software is employed to further decrease the cost of deployment.

Wireless Fidelity (Wi-Fi) utilizes unlicensed spectrum band to increase broadband internet access which can promote health care service delivery to underserved populations. The use of unlicensed frequency allows hospitals to set up links anywhere, anytime as they deem fit,

thereby improving sustainability. Large networks can be deployed with IEEE 802.11 after a little changes to the MAC layer. This will enable Wi-Fi transceivers to work effectively especially at very long distances. Cost-effective network model adopted in [30] has proven the feasibility of the deployment of Wi-Fi over Long Distances (WiLD) and femtocells in achieving broadband internet services in rural areas with acceptable Quality of Service (QoS). Wi-Fi communication technologies operate at different frequencies to deliver maximum data rates. For sustainable Internet services in third world countries, a solar-powered Wi-Fi technology will allow villagers to send signals through an IEEE 802.11 b connection [31].

Nowadays, most of the advanced technologies available to improve way of living are electricity-dependent. Unfortunately, most of the rural areas in the developing world are not connected to the power grid. For instance, in Nigeria, the majority of the less than 40% that are currently connected to the grid are located in the urban centers [32, 33]. Therefore, the system is powered by a solar photovoltaic energy source to provide a cheap and reliable power system.

III. SYSTEM IMPLEMENTATION

Figure 3 shows the implementation of the system design earlier mentioned. The total cost of the plastic mannequin-based telepresence is \$456. This is comparatively lower than existing systems, making it more affordable with satisfactory efficiency. Hence, health facilities in emerging economies can take advantage of the cost-effectiveness that this system offers to perform remote clinical ward rounding.

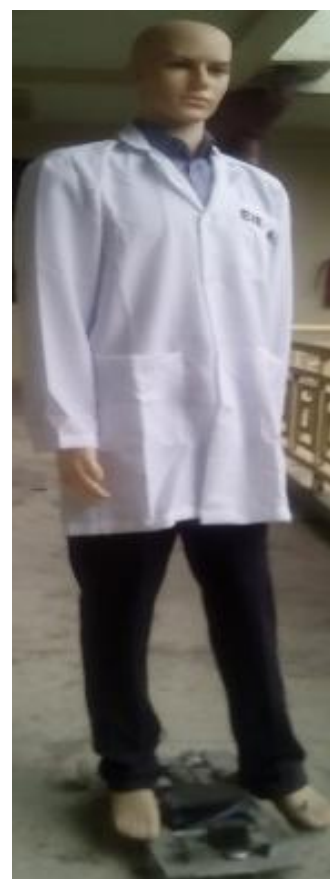


Figure 3: Plastic Mannequin-Based Robotic Telepresence

IV. CONCLUSION

Existing telepresence solutions are considered to be expensive for people living in rural areas. Most people living in rural areas, especially in emerging economies, are extremely poor and cannot afford the cost of service of a robotic telepresence. We have reduced the cost of mobile robotic telepresence solution for remote ward rounding using plastic mannequin and solar photovoltaic technology. The plastic mannequin-based telepresence utilizes two IP cameras with the ability to communicate over the Internet using Wi-Fi transceiver module available on a mini-computer. This successfully minimized the overall cost of the system. Also, the system was designed to operate on solar PV system to ensure availability of required electrical power at low cost. After a proper authentication process, a medical consultant based in any of the developed countries can easily log in to the web or mobile application platform and attend to patients in different parts of the developing countries where the mannequin robot is situated.

The developed system allows other specialists/consultants to work seamlessly with the community health workers during routine ward rounding. Patients seem to be more comfortable with a real human figure during treatment rather than relating with a typical machine appearance. In clear departure from existing robotic telepresence systems, our solution gives a better impression of the physical presence of a medical personnel. Compared to existing telepresence robot, the plastic mannequin-based system is a cost-effective, energy-efficient, and eco-friendly solution that has an enormous potential to significantly increase the adoption of robotic telepresence in rural telemedicine.

REFERENCES

- [1] World Health Organization. A health telematics policy in support of WHO's Health-For-All strategy for global health development: report of the WHO group consultation on health telematics, 11–16 December, Geneva, 1997. Geneva, World Health Organization, 1998.
- [2] Heinzlmann PJ, Lugin NE, Kvedar JC. Telemedicine in the future. *Journal of Telemedicine and Telecare*, 2005, 11(8):384–390.
- [3] Craft RL: Trends in technology and the future intensive care unit. *Crit Care Med* 29S:N151-N158, 2001
- [4] Poropatich RK, DeTreville R, Lappan C, et al: The U.S. Army telemedicine program: General overview and current status in Southwest Asia. *Telemed J E Health* 12:396-408, 2006
- [5] Grundy BL, Crawford P, Jones PK, et al: Telemedicine in critical care: an experiment in health care delivery. *JACEP* 6:439-444, 1977
- [6] Grundy BL, Jones PK, Lovitt A: Telemedicine in critical care: Problems in design, implementation and assessment. *Crit Care Med* 10:471-475, 1982
- [7] Celi LA, Hssan E, Marquardt C, et al: The eICU: It's not just telemedicine. *Crit Care Med* 29S:N183-N189, 2001.
- [8] Rosenfeld BA, Dorman T, Breslow MJ, et al: Intensive care unit telemedicine: Alternate paradigm for providing continuous intensive care. *Crit Care Med* 28:3925-3931, 2000.
- [9] Breslow MJ, Rosenfeld BA, Doerfler M, et al: The effect of a multi-site ICU telemedicine program on clinical and economic outcomes: An alternative paradigm for intensivist staffing. *Crit Care Med* 32:31-38, 2004
- [10] Ricci MA, Caputo M, Amour J, et al: Telemedicine reduces discrepancies in rural trauma care. *Telemed J E Health* 9:3-11, 2003
- [11] LaMonte MP, Bahouth MN, Hu P, et al: Telemedicine for acute stroke: Triumphs and pitfalls. *Stroke* 34:725-728, 2003
- [12] Shwamm LH, Rosenthal ES, Hirshberg A, et al: Virtual TeleStroke support for the emergency department evaluation of acute stroke. *Acad Emerg Med* 11:1193-1197, 2004

- [13] Ickenstein GW, Horn M, Schenkel J, et al: The use of telemedicine in combination with a new stroke-code-box significantly increases t-PA use in rural communities. *Neurocrit Care* 3:27-32, 2005
- [14] Audebert HJ, Kukla C, Clarmann von Claranau S, et al: Telemedicine for safe and extended use of thrombolysis in stroke: The Telemed Pilot Project for Integrative Stroke Care (TEMPiS) in Bavaria. *Stroke* 36:287-291, 2005
- [15] Craig J, Patterson v. Introduction to the practice of telemedicine. *Journal of Telemedicine and Telecare*, 2005, 11(1):3–9.
- [16] Al Shorbaji N. e-Health in the Eastern Mediterranean region: A decade of challenges and achievements. *East Mediterranean Health Journal*, 2008, 14(Supp.):S157–S173.
- [17] Kifle M, Mbarika V, Datta P. Telemedicine in sub-Saharan Africa: The case of teleophthalmology and eye care in Ethiopia. *Journal of the American Society for Information Science & Technology*, 2006, 57(10):1383–1393.
- [18] Swanepoel D, Olusanya B, Mars M. Hearing health-care delivery in sub Saharan Africa – a role for tele-audiology. *Journal of Telemedicine and Telecare*, 2010, 16(2):53–56.
- [19] Ellison LM, Pinto PA, Kim F, et al. Telerounding and patient satisfaction after surgery. *J Am Coll Surg* 2004;199:523–30.
- [20] Thacker PD. Physician-robot makes the rounds. *JAMA* 2005;293:150.
- [21] Vespa P. Robotic telepresence in the intensive care unit. *Crit Care*, 2005;9:319–20.
- [22] Vespa PM, Miller C, Hu X, et al. Intensive care unit robotic telepresence facilitates rapid physician response to unstable patients and decreased cost in neurointensive care. *Surg Neurol* 2007;67:331–7.
- [23] Gandsas A, Parekh M, Bleech MM, et al. Robotic telepresence: profit analysis in reducing length of stay after laparoscopic gastric bypass. *J Am Coll Surg* 2007;205:72–7.
- [24] Chung KK, Grathwohl KW, Poropatich RK, et al. Robotic telepresence: past, present, and future. *J Cardiothorac Vasc Anesth* 2007; 21: 593–6.
- [25] Manecke GR Jr. Editorial: robotics and telepresence—the future is arriving ahead of schedule. *J Cardiothorac Vasc Anesth* 2007;21:592.
- [26] Ellison LM, Nguyen M, Fabrizio MD, et al. Postoperative robotic telerounding: a multicenter randomized assessment of patient outcomes and satisfaction. *Arch Surg* 2007;142:1177–81.
- [27] P. D. Z. Varcheie and G. A. Bilodeau, "Adaptive Fuzzy Particle Filter Tracker for a PTZ Camera in an IP Surveillance System," in *IEEE Transactions on Instrumentation and Measurement*, vol. 60, no. 2, pp. 354-371, Feb. 2011.
- [28] M. J. Yang, J. Y. Tham, D. Wu and K. H. Goh, "Cost effective IP camera for video surveillance," 2009 4th IEEE Conference on Industrial Electronics and Applications, Xi'an, 2009, pp. 2432-2435.
- [29] G. Bekaroo and A. Santokhee, "Power consumption of the Raspberry Pi: A comparative analysis," 2016 IEEE International Conference on Emerging Technologies and Innovative Business Practices for the Transformation of Societies (EmergiTech), Mauritius, 2016, pp. 361-366. doi: 10.1109/EmergiTech.2016.7737367
- [30] TUCAN3G Project. [Online] Available: <http://www.ict-tucan3g.eu/>
- [31] K.R. Santhi and G. Senthil Kumaran, Solar Powered Wi-Fi with Wimax Enables Third World Phones, In Proceedings from the International Conference on Advances in Engineering and Technology, edited by J.A. Mwakali and G. Taban-Wani, Elsevier Science Ltd, Oxford, 2006, Pages 635-646
- [32] UN. World urbanization prospects: the 2014 revision, highlights (ST/ESA/SER.A/352); 2014.
- [33] Melodi Adegoke Oladipo, Temikotan Kehinde Olusesan. A Model Unavailability Perspective of Existing Nigerian Township Electricity Distribution. *International Journal of Electrical and Computer Engineering (IJECE)*, vol. 7, No. 1, February, 2017.